

FIG. 1

10036828 122101

Fig. 2A


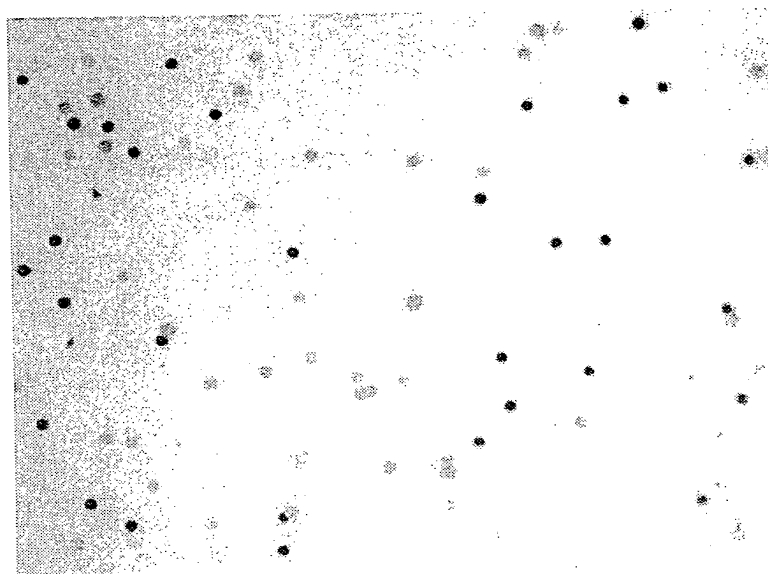


Fig. 2B

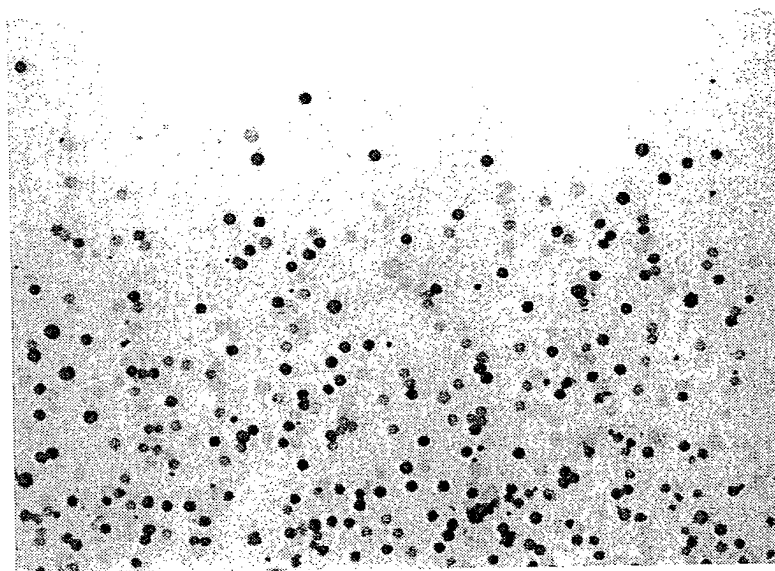

10036828 122101

Fig. 3A


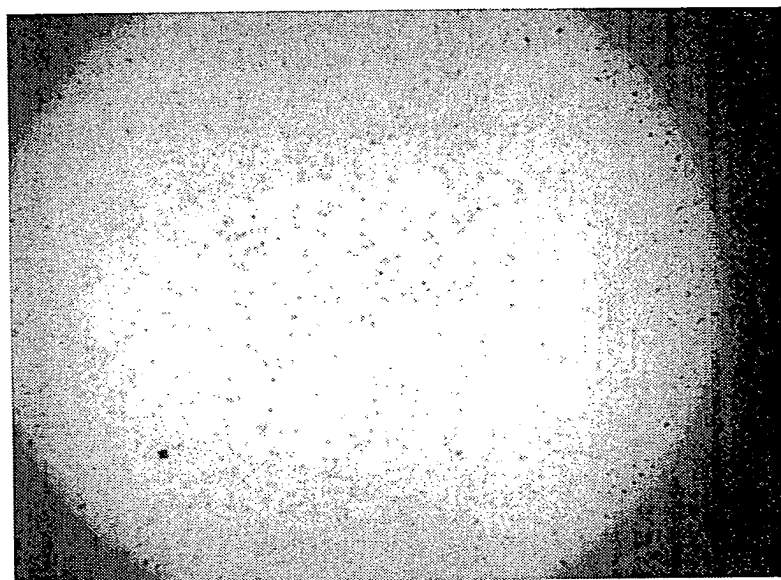


Fig. 3B

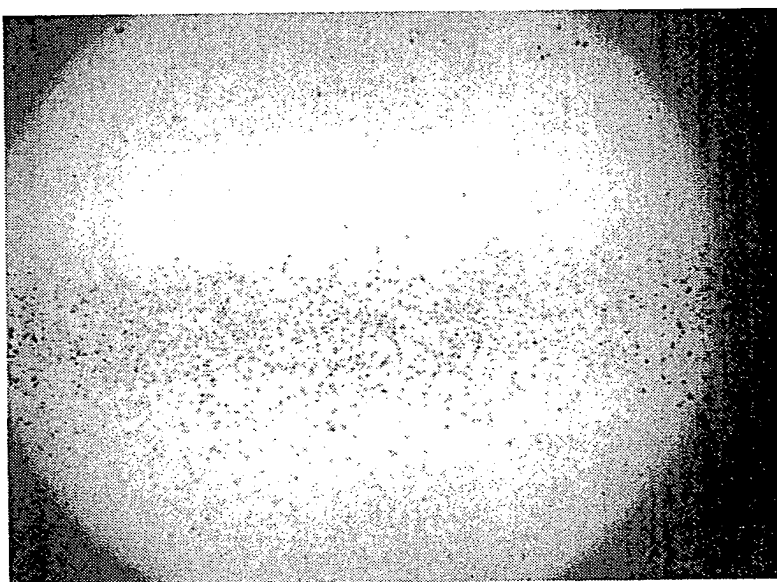

10036828 122101

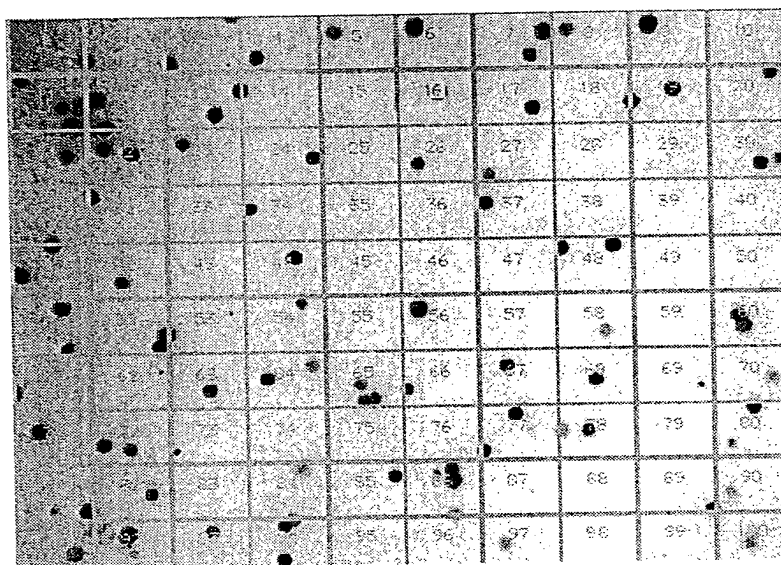


FIG. 4A

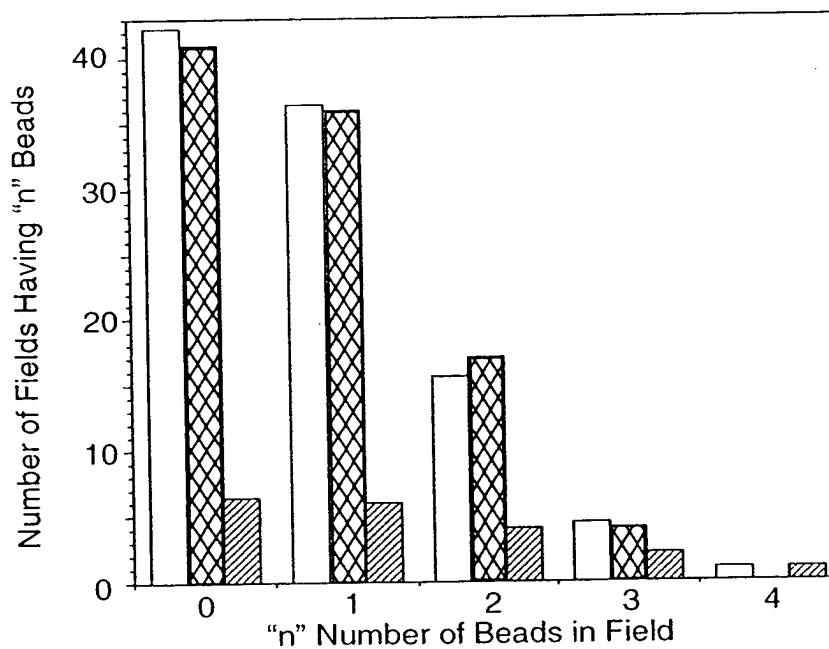


FIG. 4B

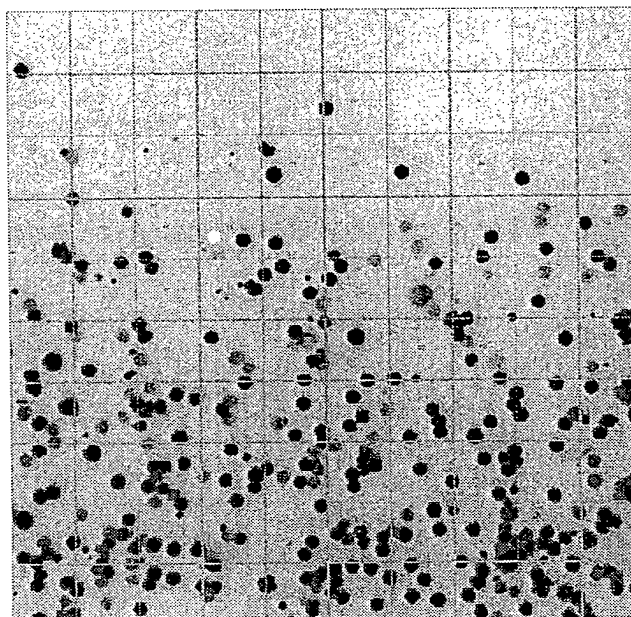


Fig. 5A

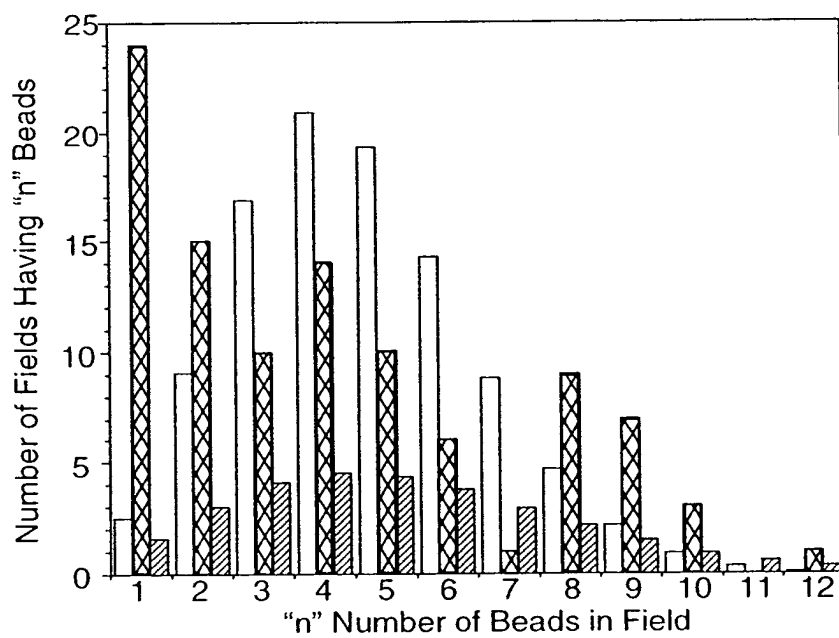


Fig. 5B

Description of Schematic

Diagram

- A. Color Beads DNA Microarray
- B. Illumination light source
- C. Cover Lid
- D. Light Deflector
- E. Lens
- F. Charge Coupled Device (CCD) Camera
- G. Computer control unit


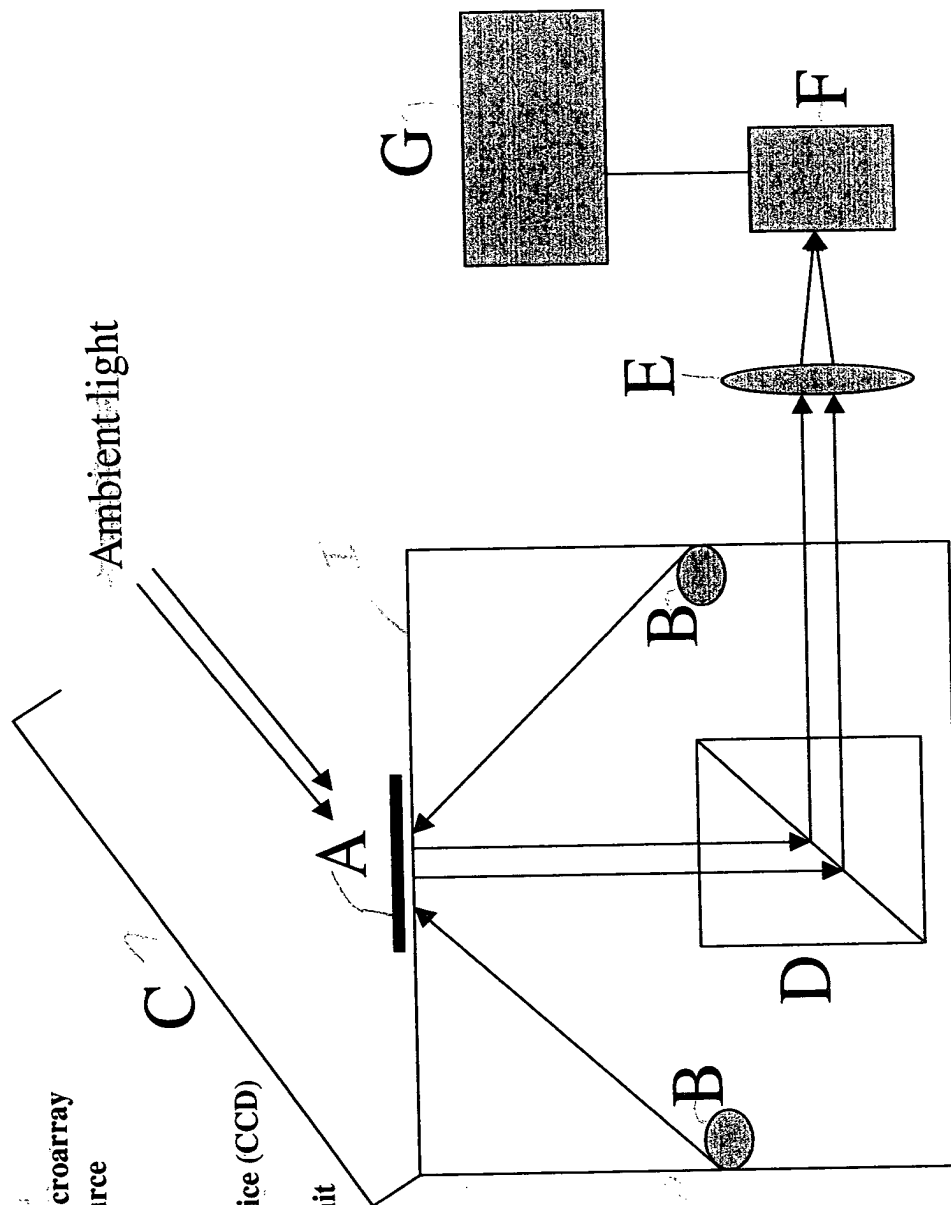


Fig. 7.

Workflow Chart of Nucleic Acid Random Microarray Analysis System

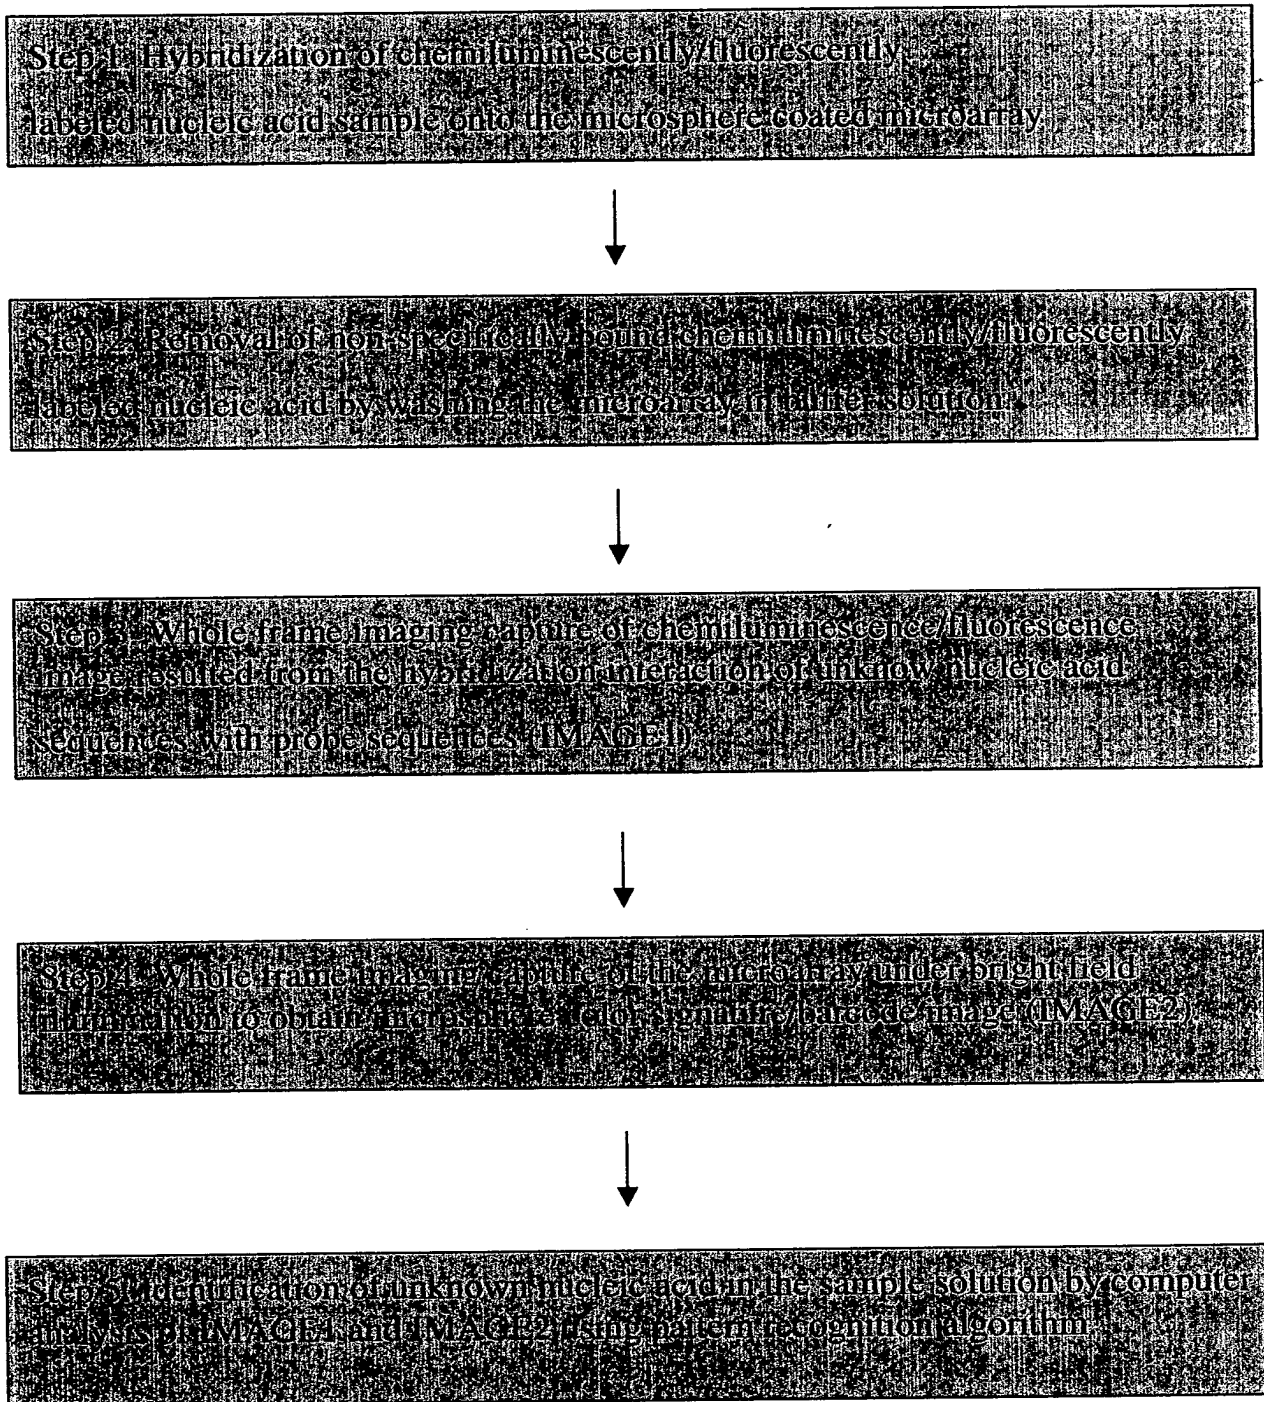

10036828-122101

Fig 8 A

10036828-122101

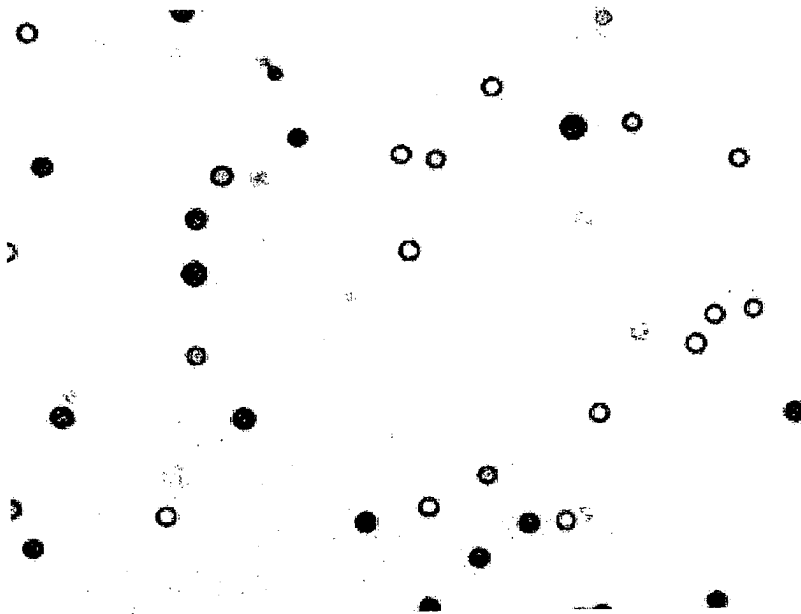


Fig 8 B

10036828.122101



Fig 9A

10036028 122101

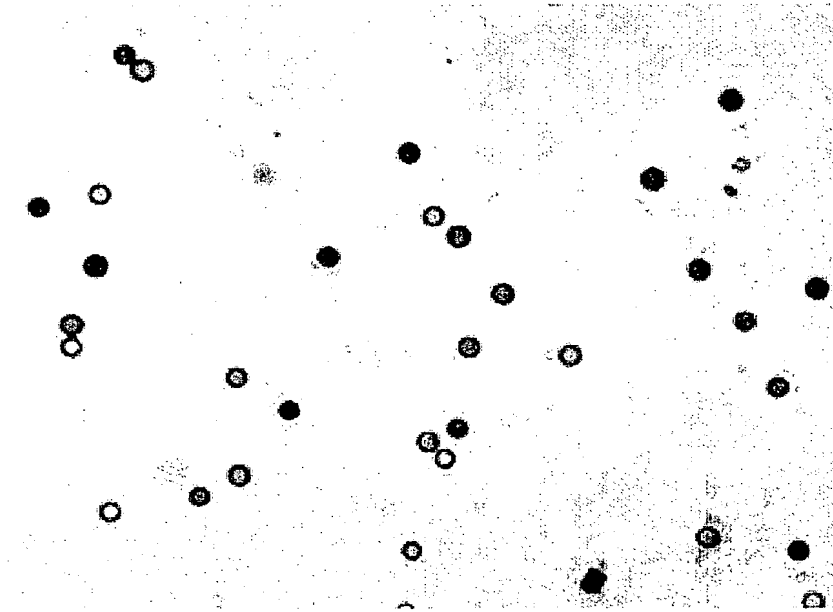


Fig 9 B



10036828-122101

10036828-122101

